



Microplate, 1536-well 781640

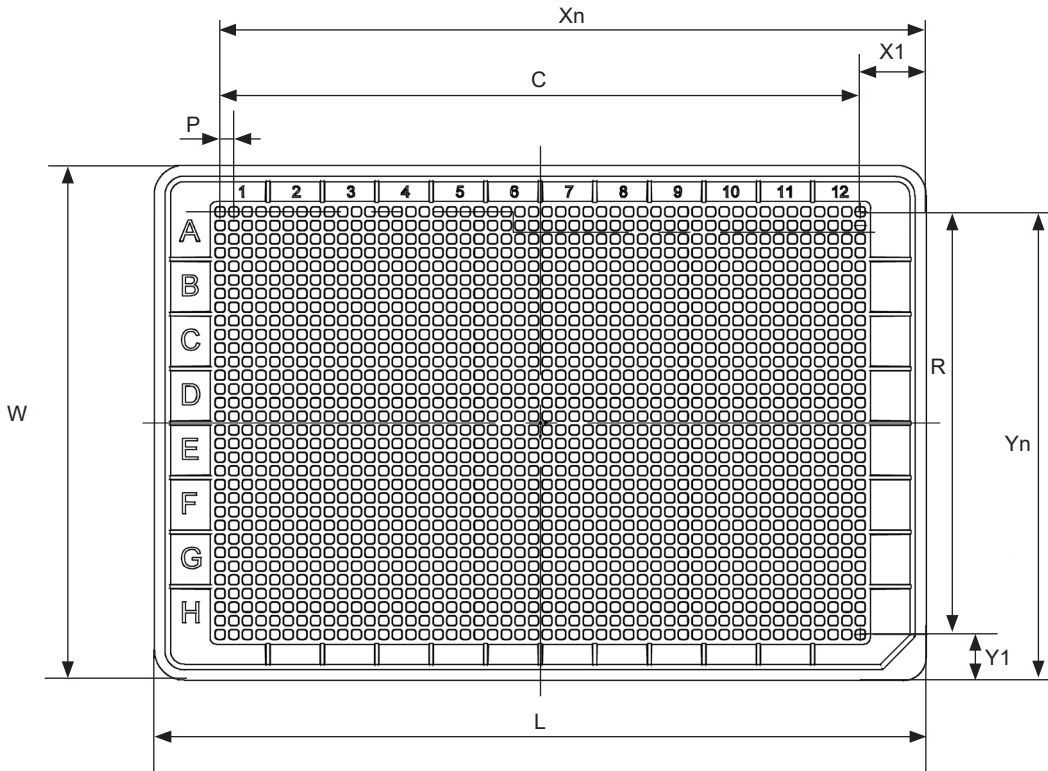

L	127.76 mm
W	85.45 mm
H	10.00 mm
Hs	2.90 mm
X1	10.88 mm
Xn	116.63 mm
Y1	7.63 mm
Yn	77.38 mm
P	2.25 mm
D	1.70 mm
Hw	5.00 mm
C	48 Well
R	32 Well

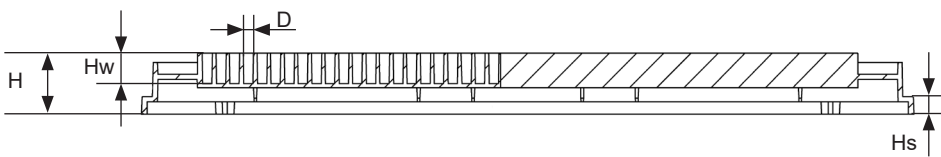


Type	standard
Base shape	F-bottom
Surface	pureGrade™
Volume	10 µl / well
Material	PS
Color	transparent
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of cytotoxic substances acc. ISO 10 993-5




* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

Microplate, 1536-well 781641

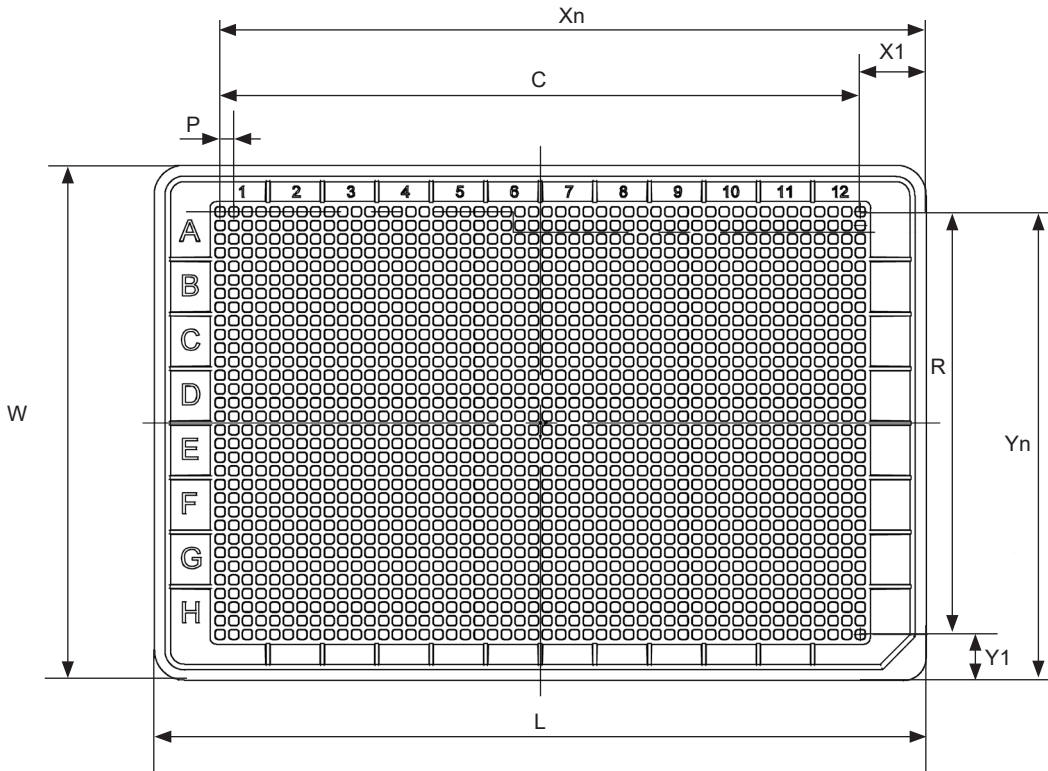

L	127.76 mm
W	85.45 mm
H	10.00 mm
Hs	2.90 mm
X1	10.88 mm
Xn	116.63 mm
Y1	7.63 mm
Yn	77.38 mm
P	2.25 mm
D	1.70 mm
Hw	5.00 mm
C	48 Well
R	32 Well

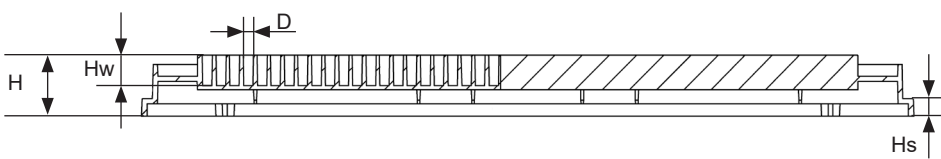


Type	standard
Base shape	F-bottom
Surface	pureGrade™
Volume	10 µl / well
Material	PS
Color	white
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of cytotoxic substances acc. ISO 10 993-5




* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

Microplate, 1536-well 781642

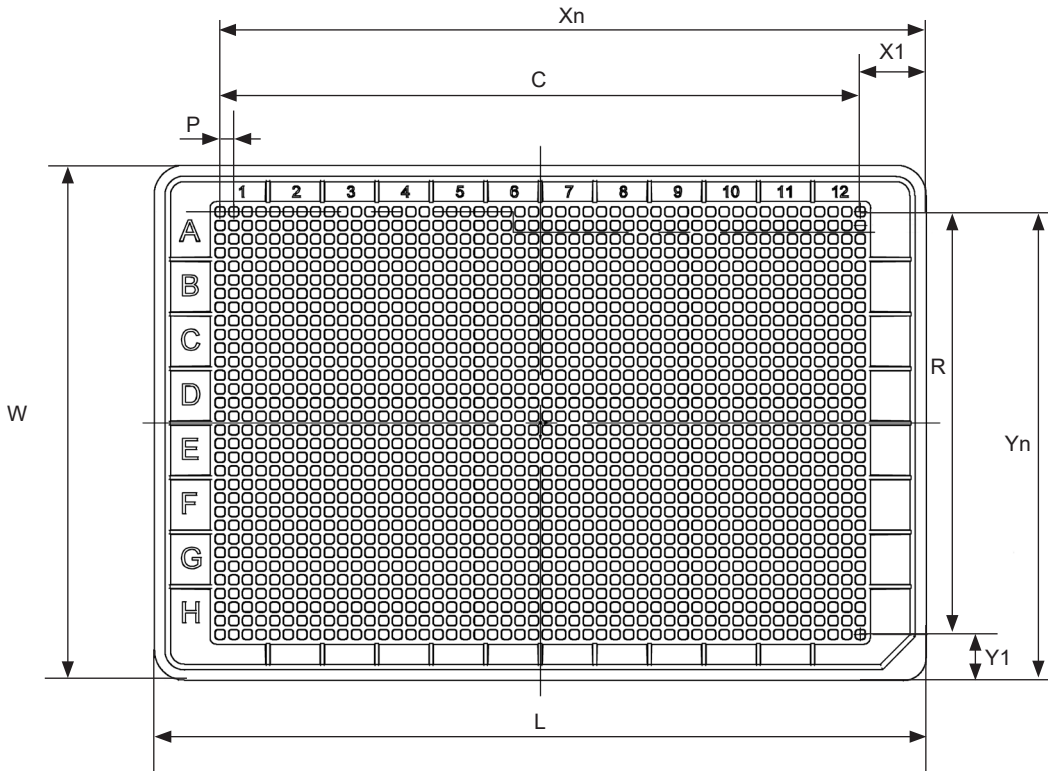

L	127.76 mm
W	85.45 mm
H	10.00 mm
Hs	2.90 mm
X1	10.88 mm
Xn	116.63 mm
Y1	7.63 mm
Yn	77.38 mm
P	2.25 mm
D	1.70 mm
Hw	5.00 mm
C	48 Well
R	32 Well

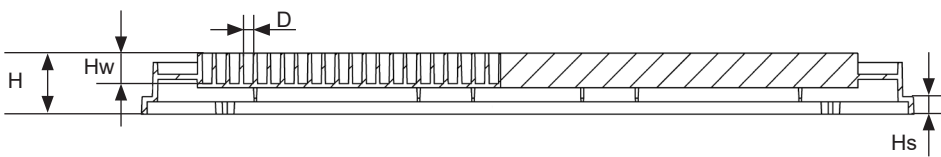

Type	standard
Base shape	F-bottom
Surface	pureGrade™
Volume	10 µl / well
Material	PS
Color	black
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of cytotoxic substances acc. ISO 10 993-5



* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.